


Supplementary material

Kempa M, Sławiński G, Zieleniewicz P, et al. Optimizing sudden cardiac death prevention: a promise of wearable cardioverter-defibrillator. *Pol Arch Intern Med.* 2024; 134: 16675. doi:10.20452/pamw.16675

Please note that the journal is not responsible for the scientific accuracy or functionality of any supplementary material submitted by the authors. Any queries (except missing content) should be directed to the corresponding author of the article.

Supplementary Figure S1 Clinical outcomes following wearable cardioverter-defibrillator monitoring completion

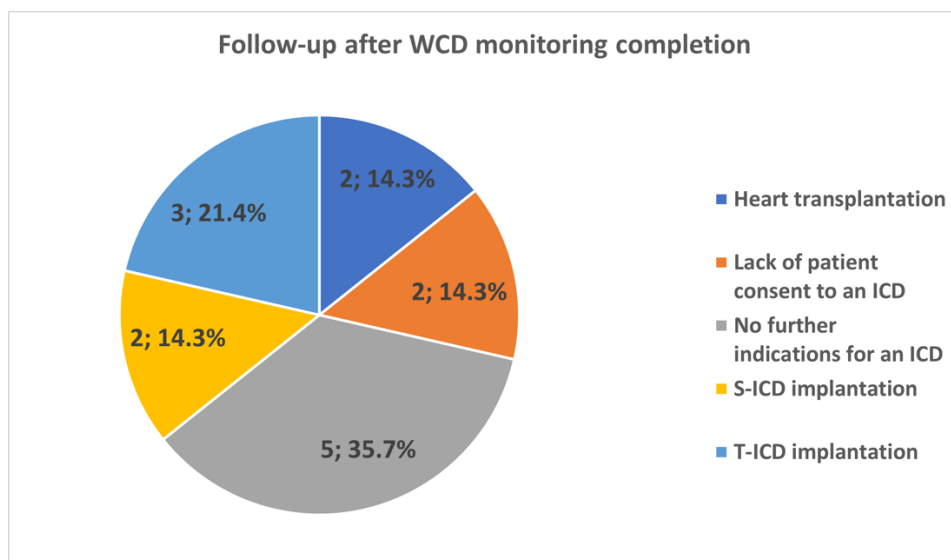

Supplementary Figure S2 Recordings from a wearable cardioverter-defibrillator; **A** – nonsustained ventricular tachycardia; **B** – sustained ventricular tachycardia; **C** – artifacts

